Silverback Wellness

CERTIFICATE OF ANALYSIS · LOT RELEASE

silverbackgroup.co

CERTIFICATE NO.
PL–26–00036

VERIFICATION KEY
722T4EGC

Scan or enter both at prymalab.net/testing/verify

CERTIFICATE OF ANALYSIS · LOT RELEASE · ISSUED FOR SILVERBACK WELLNESS

GHK-Cu 100 mg

Lot **PL-2609-036** · Lyophilized powder · Label claim **100 mg/vial** · Distributed as **GHK-Cu**

TESTED IN-HOUSE BY PRYMALAB

In-house analytical result, not an independent third-party test

LOT / BATCH NUMBER	DATE MADE	DATE OF ANALYSIS	DATE ISSUED
PL–2609–036	**2026-09-16**	**2026-09-18**	**2026-10-03**
RETEST / EXPIRY	**UNITS IN LOT / SAMPLED**	**STORAGE**	**CERTIFICATE TYPE**
2028-09-16	**250 / 2**	−20 °C, desiccated, dark	Lot COA, 2 pages

COMPOUND	CAS NUMBER	MOLECULAR FORMULA	THEORETICAL MASS (AVG.)
GHK-Cu Copper tripeptide-1; Gly-His-Lys · Cu(II)	**89030-95-5**	$C_{14}H_{22}CuN_6O_4$	401.9 Da

SEQUENCE

`H–GHK–OH · Cu(II) (1:1 complex; copper bound by the Gly α–amine, the Gly–His amide nitrogen and the His imidazole)`

PURITY · RP-HPLC, AREA %
99.62%
Specification 99.0% • main peak at 2.20 min


IDENTITY · OBSERVED MASS
402.1 Da
Theoretical 401.9 Da • +0.2 Da (498 ppm)

OVERALL CONCLUSION
PASS
Meets every specification for the tests performed

TEST	METHOD	SPECIFICATION	RESULT	CONCLUSION
Appearance	Visual inspection	Blue to blue-violet lyophilized powder	Blue lyophilized powder	**PASS**
Identity (mass)	LC-MS, ESI positive	Theoretical ± 1.0 Da	402.1 Da	**PASS**
Purity	RP-HPLC, UV 214 nm, area%	99.0%	99.62%	**PASS**
Largest impurity	RP-HPLC, area%	1.0%	0.21% at 1.94 min (free-GHK dissociation)	**PASS**
Water content	Karl Fischer	5.0%	2.0%	**PASS**
Bacterial endotoxin	LAL, kinetic	≤ 5.0 EU/mg	0.04 EU/mg	**PASS**
Sterility / bioburden	USP <71>, membrane filtration	No growth after 14 days	No growth; conforms	**PASS**

1 HPLC CHROMATOGRAM

Data file: GHK_PL-2609-036_20260918_01 · Column C18, 150 × 4.6 mm · UV 214 nm

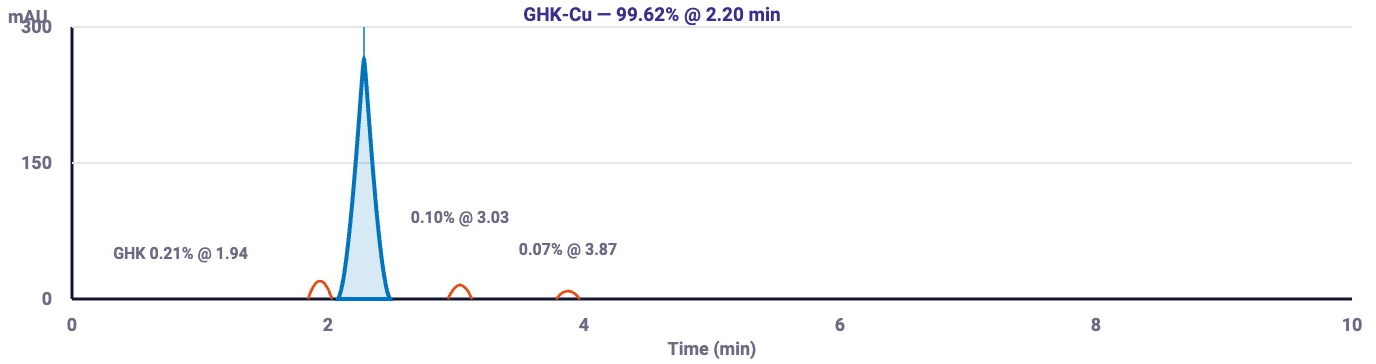

Baseline uncropped; main peak, free-GHK dissociation peak, and impurities labeled with retention times. Peak table on page 2.

For laboratory research use only. Not for human or veterinary use.

2 HPLC METHOD · GHK_PL-2609-036_20260918_01

INSTRUMENT Waters Alliance e2695, SN E2695B742	DATA SYSTEM Empower 3, Build 3471	DETECTOR Waters 2998 PDA
DETECTION WAVELENGTH 214 nm	COLUMN C18, 150 × 4.6 mm, 3.5 µm	COLUMN PART / SERIAL 18600003326 / USHX18211
MOBILE PHASE A 0.1% TFA in water	MOBILE PHASE B 0.1% TFA in MeCN	FLOW RATE 1.0 mL/min
COLUMN TEMPERATURE 30 °C	INJECTION VOLUME 20 µL	RUN TIME 10 min
SAMPLE DILUENT Water, 0.1% TFA	SAMPLE CONCENTRATION 0.5 mg/mL	BLANK INJECTED Yes

REFERENCE STANDARD

In-house GHK-Cu reference, lot PL-RS-GHK-01, RT 2.18 min (GHK reference, RT 1.92 min)

3 GRADIENT PROGRAM

TIME (MIN)	% A	% B
0.0	95	5
3.0	95	5
7.0	55	45
8.0	20	80
9.0	20	80
10.0	95	5

4 PEAK TABLE

PEAK	RT (MIN)	AREA	AREA %
1 (free GHK)	1.94	9,030	0.21
2 (GHK-Cu)	**2.20**	**4,283,660**	**99.62**
3	3.03	4,300	0.10
4	3.87	3,010	0.07
Total		4,300,000	100.00

Threshold 0.05% area · Blank subtracted: Y · Purity = main peak area ÷ total integrated area × 100, to two decimals; main peak shaded.

5 IDENTITY BY MASS SPECTROMETRY

INSTRUMENT Waters Acquity SQD	IONIZATION / MODE ESI, positive	OBSERVED M/Z (CHARGE) 402.8 (1+ [M+H]) · 424.8 (1+ [M+Na])
DECONVOLUTED MASS 402.1 Da	THEORETICAL MASS 401.9 Da	DIFFERENCE +0.2 Da (498 ppm)
DATA FILE GHK_PL-2609-036_MS_20260918_01	ACCEPTANCE Within ± 1.0 Da	

6 ADDITIONAL TESTS

TEST	PERFORMED BY	DATE	REPORT / FILE
Water content	PrymaLab	2026-09-19	RPT-KF-PL-2609-036
Endotoxin	PrymaLab	2026-09-20	RPT-ET-PL-2609-036
Sterility	PrymaLab	2026-10-02	RPT-ST-PL-2609-036
Peptide content	PrymaLab	2026-09-19	RPT-AA-PL-2609-036

A test with no row here was not performed on this lot. Outside-laboratory reports, when used, are attached and named below.

7 REVIEW AND APPROVAL

D. Reynolds
Analyst · performed the testing
Date: 2026-09-18

S. Calloway
Reviewer · checked against raw data
Date: 2026-10-02

M. Phelps
Lab Director · approved for release
Date: 2026-10-03

Raw data retained at: Empower 3 (Build 3471), project PL-2609, archive PL-ARC-2026; 7 years. Outside laboratory reports attached: None

This certificate applies only to the lot named above and describes the units sampled from it; it is not a guarantee for any other lot. Results were obtained by PrymaLab LLC's own laboratory (PrymaLab Analytical) and are not an independent third-party test unless an outside report is attached. This copy is issued for Silverback Wellness, a distributor of the lot; the brand shown does not change the laboratory, the method or the results. Reference values (CAS, formula, theoretical mass, sequence) are literature values for the named compound. Authenticity: scan the QR code or enter certificate number PL-26-00036 and key 722T4EGC at prymalab.net/testing/verify; any copy that does not match the record shown there is not a PrymaLab certificate. PrymaLab LLC products are supplied for laboratory research use only and not for human or veterinary use.